



Accessories


- Monitor with adjustable neck strap and fitted batteries (with integrated position sensor)
- Adjustable chest strap (long) and arm strap (short) for attachment
- Oxygen saturation sensor with plugged-in connection cable
- Patient record and instructions
- Closure tape for return

Return

After completing the recording, please return the monitor to us by mail with plugged-in cables, belts, arm strap, position sensor, oxygen saturation sensor, and patient record

Please follow the instructions for the return of the box:

- Remove the label from the window, turn it over
→ **Viollier AG address is visible**
- Insert the label into window
- Close the box with the enclosed closure tape
- Viollier will pay the postage

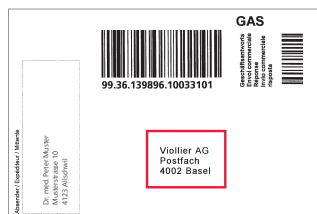

IN STRUCTION



Nocturnal pulse oximetry

With CPAP treatment



Important information

You should wear your CPAP mask while recording. Please send your CPAP chip back to us along with the monitor. Your CPAP monitor will also work without a chip.

Do not test start the monitor → monitor can not be switched off again.

- Remove nail polish or fingernail attachments before the examination.
- Do not put the oxygen saturation sensor on the same limb as the 24h blood pressure monitor cuff if these two devices are worn at the same time.
- Mount and start the monitor before going to bed.
- Recording time max. 8 hours, suitable for patients weighing 20 kg and over.
- Leave batteries in the monitor; do not remove.
- Do not use in the vicinity of CT, MRI and X-rays.
- Mobile phones, strong electromagnetic sources, and electric blankets can affect the quality of the recording.




Patient record

Please complete the patient record accurately and in full.

Note start and end of recording with date and time.

[illegible]

Attaching the monitor

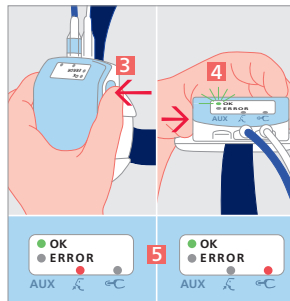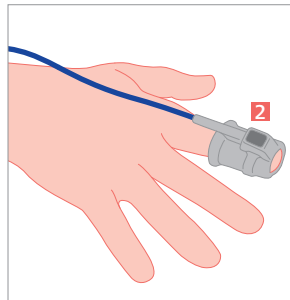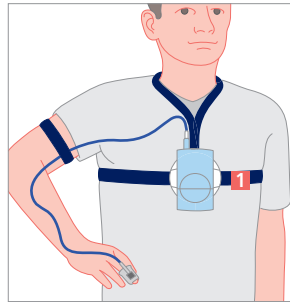

Mounting the monitor before going to bed

- Do not wear the monitor and the chest strap directly on the skin.
- Pull the neck strap and the monitor over the head and pull the chest strap through the monitor holder.
- Fix the monitor with the chest strap 1 centrally at the height of sternum → for men at nipple level, for women on the upper part of the chest.
- Tighten the strap, but not so much that breathing is restricted.

Fitting the finger sensor

- Fit the oxygen saturation sensor to your finger with the fingernail symbol facing upward. Pull the finger sensor over the finger until the fingertip is visible.
→ The finger sensor **2** may be switched from one finger to another during the night.
- Suitable are: index, middle and ring finger (without nail polish).
- Attach sensor cable to the upper arm with the arm strap.

Starting the monitor

- Hold down the side **light blue start button** **3** for five seconds until a short beep tone sounds, and on the display a **green flashing light** **4** appears in the 'OK' field.
- Ignore the red light in the middle.
- If the finger sensor is released at night, please remount **5**.
- In the morning dismount the monitor and return. Monitor switches off automatically after 8 hours.

Solely on behalf of the physician

- Please attach the enclosed T-adapter piece between the mask and the tube. Then insert the CPAP sensor into the middle socket of the adapter.